


**HPLC**

Order ID USCLBPC745370  
 Lot. No BPC00210 – BPC00255  
 Pump A 0.1% trifluoroacetic in 100% water  
 Pump B 0.1% trifluoroacetic in 100% acetonitrile  
 Total Flow 0.8ml/min  
 Wavelength 220nm  
 Analytical column type Phenomenex Luna 3um C18 (2) (4.6\*150mm\*3um)  
 Dissolution method 100% H<sub>2</sub>O  
 Acquisition Time 5/12.2024  
 Inj. Volume 20ul

Time	Module	Action	Value
0.01	Pumps	B.Conc	12
25	Pumps	B.Conc	37
30	Pumps	B.Conc	90
31	Controller	Stop	

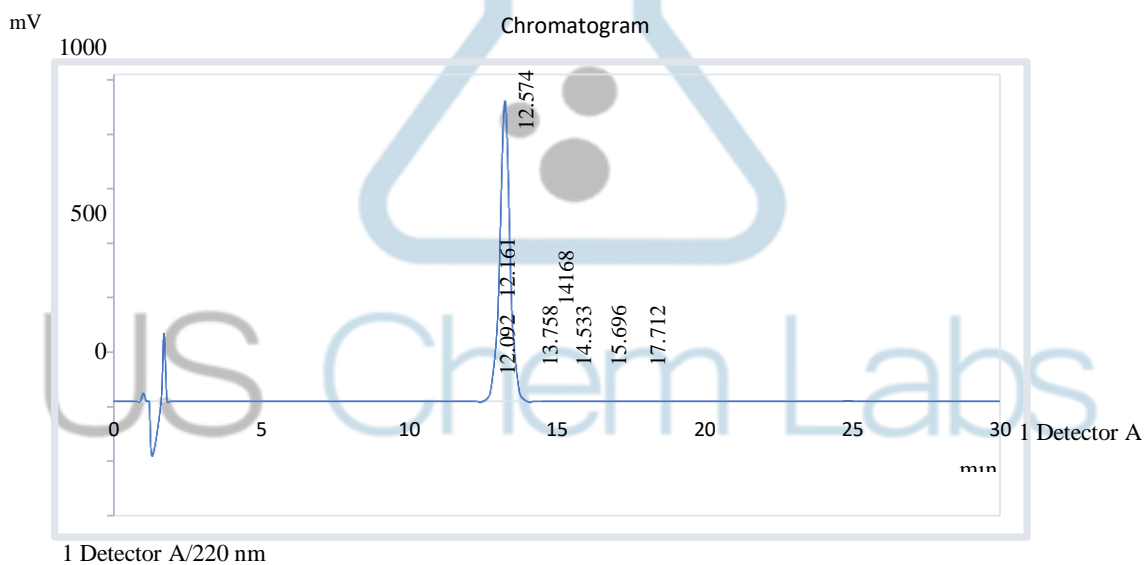

**PeakTable**

Detector A 220nm

Peak#	Ret. Time	Area	Height	Area %
1	12.092	82506	9377	0.202
2	12.161	94195	10466	0.203
3	12.574	16135827	808939	99.015
4	13.754	8990	868	0.055
5	14.168	69399	4399	0.212
6	14.533	8534	742	0.042
7	15.696	17833	1319	0.201
8	17.712	11707	954	0.065
Total		16428991	837064	100.00