


HPLC

Order ID: USLCTESA12030
 Lot. No: TES00190 - TES00205
 Pump A: 0.1% trifluoroacetic in 100% water
 Pump B: 0.1% trifluoroacetic in 100% acetonitrile
 Total Flow: 0.8ml/min
 Wavelength: 220nm
 Analytical column type: Phenomenex Luna 3um C18 (2) (4.6*150mm*3um)
 Dissolution method: 100% H₂O
 Acquisition Time: 5/21/2024
 Inj. Volume: 40ul

Time	Module	Action	Value
0.01	Pumps	B.Conc	30
25	Pumps	B.Conc	45
30	Pumps	B.Conc	90
31	Controller	Stop	

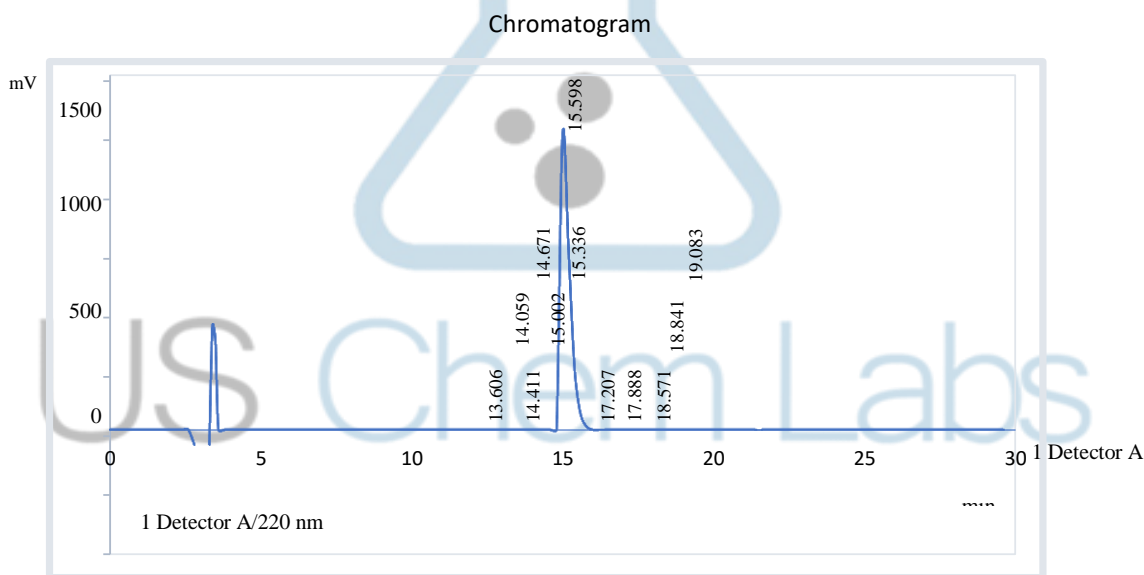

PeakTable

Detector A 220nm

Peak#	Ret. Time	Area	Height	Area %
1	13.606	2461	343	0.011
2	14.059	51557	4436	0.110
3	14.411	40126	3258	0.186
4	14.671	64560	5119	0.175
5	15.002	16357	1650	0.072
6	15.336	55384	4959	0.257
7	15.598	21308602	908927	99.018
8	17.207	5585	596	0.026
9	17.888	12884	1097	0.060
10	18.571	5829	568	0.027
11	18.841	10080	993	0.047
12	19.083	2512	305	0.012
Total		21575937	932251	100.000