


## HPLC

Order ID: USCLSEMA10129  
 Lot. No: SEM05690 - SEM05725  
 Pump A: 0.1% trifluoroacetic in 100% water  
 Pump B: 0.1% trifluoroacetic in 100% acetonitrile  
 Total Flow: 0.8ml/min  
 Wavelength: 220nm  
 Analytical column type: 3u C18 (2) (4.6\*150mm\*3um)  
 Dissolution method: 100% H<sub>2</sub>O  
 Acquisition Time: 7/2/2024  
 Inj. Volume: 15ul

Time	Module	Action	Value
0.01	Pumps	B.Conc	45
25.00	Pumps	B.Conc	70
30.00	Pumps	B.Conc	90
31.00	Controller	Stop	

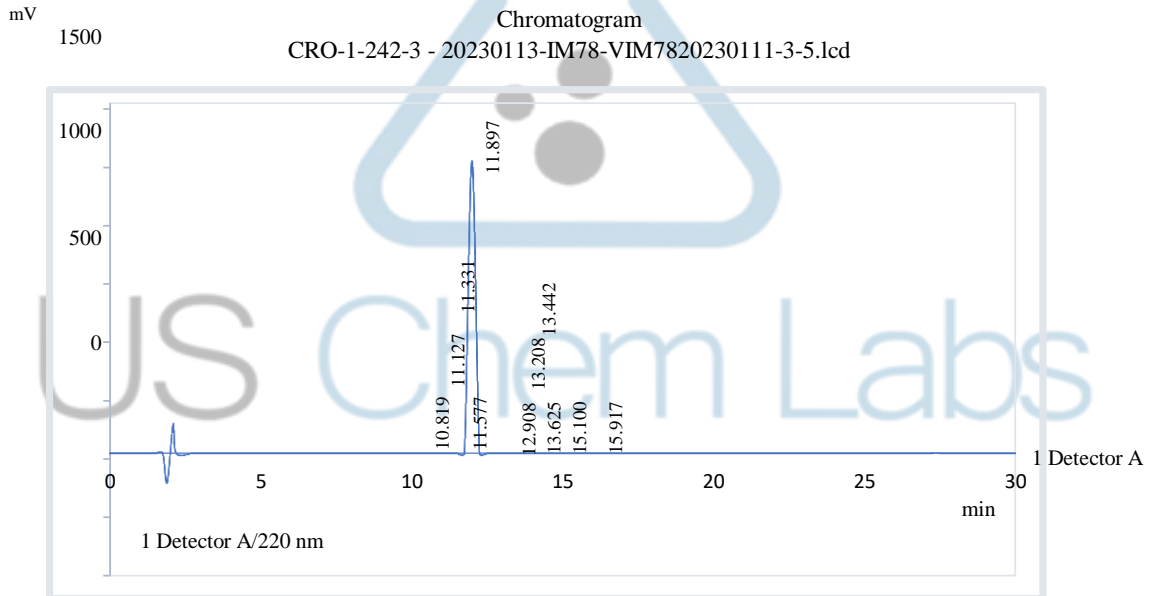

### PeakTable

Detector A 220nm

Peak#	Ret. Time	Area	Height	Area %
1	10.819	9642	955	0.097
2	11.127	7268	1168	0.073
3	11.331	13349	1816	0.134
4	11.577	41946	3541	0.422
5	11.897	9865824	1014126	<b>99.156</b>
6	12.908	1536	223	0.015
7	13.208	4668	386	0.047
8	13.442	2189	349	0.022
9	13.625	1158	133	0.012
10	15.1	1005	166	0.010
11	19.917	1242	210	0.012
Total		9949827	1023073	100.000