


**MS Spectrum**

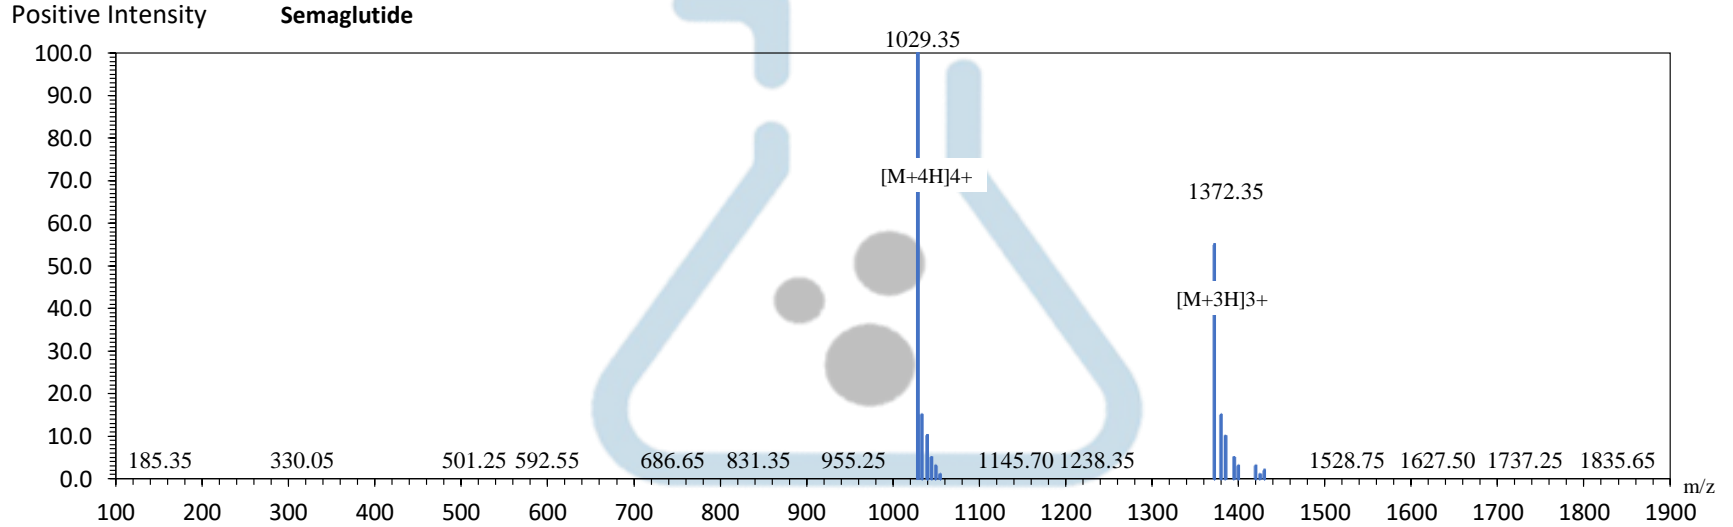

**Sample Information**

Dissolution method : 3% HAC+25%ACN+72%H<sub>2</sub>O  
Date Acquired : 2024/5/2 13:45:52  
Injection Volume : 1ul

Interface : ESI  
Nebulizing Gas Flow : 1.50L/min  
CDL Temp : 250C  
CDL Volt : 0v  
Block Temp : 200  
Perod Bias : +4.5kv  
Detector : -0.2kv  
T.Flow : 0.2ml/min  
B.conc : 30%H<sub>2</sub>O/70%MeOH

Lot No.	SEM05690 - SEM05725
Item ID:	USCLSEMA10129
Date Acquired:	7/2/2024
Theoretical	4113.6
Observed	4113.4